

Certificate number: o60235225i286640-A-1



Calibration Certificate



Customer
PHYSICS ASSOCIATES LLC
PETERS CREEK RD 5346
24019 ROANOKE
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

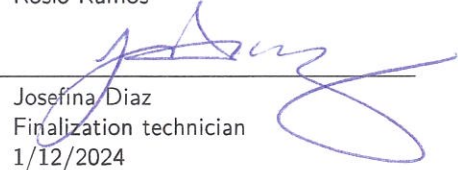
CUSTOMER INSTRUMENT

Product X2 MAM
Serial number 286640
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 1/9/2024
As left 1/11/2024
Adjustment done Yes
Tested by Christina Arroyo
Rosio Ramos

Approved by


Josefina Diaz
Finalization technician

Certificate date 1/12/2024

CALIBRATION RESULT

AS FOUND: One or more measured and tested values of this certificate are within the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state conformance with specifications for those measurements.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air Kerma: 5 %
Voltage: 2 % or 0.5 kV (without paddle), 2 % or 0.7 kV (with paddle)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Calibration Certificate



Customer
PHYSICS ASSOCIATES
PETERS CREEK RD NW 5346
24019 ROANOKE
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

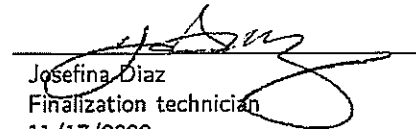
CUSTOMER INSTRUMENT

Product X2 mAs
Serial number 282198
Manufacturer RaySafe

CALIBRATION INFORMATION

As found Not performed
As left 11/17/2022
Adjustment done Yes
Tested by Channell Kennedy

Approved by


Josefina Diaz
Finalization technician

Certificate date 11/17/2022

CALIBRATION RESULT

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Electrical charge: 1 %
Electrical current: 1 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Calibration Certificate



Customer
PHYSICS ASSOCIATES
PETER CREEK RD 5346
24019 ROANOKE
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 267472
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 11/3/2023
As left 11/3/2023
Adjustment done Yes
Tested by Tommy Cox

Approved by

Josefina Diaz
Finalization technician
Certificate date 11/8/2023

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %, Air kerma rate: 5 %
Time: 0.5 %, Voltage: 2 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.

